

ASSEMBLY INSTRUCTION

UPMGV-04 Ultimate Premium Masterline Bioboosted Armor Guyver Guyver III



REMOVAL INSTRUCTIONS




PRIME1
STUDIO
<https://www.prime1studio.co.jp>
<https://www.instagram.com/Prime1Studio>
<https://twitter.com/Prime1Studio>
<https://www.facebook.com/Prime1Studio>

© 高屋良樹 / KADOKAWA

ASSEMBLY INSTRUCTION

UPMGV-04 Ultimate Premium Masterline Bioboosted Armor Guyver Guyver III

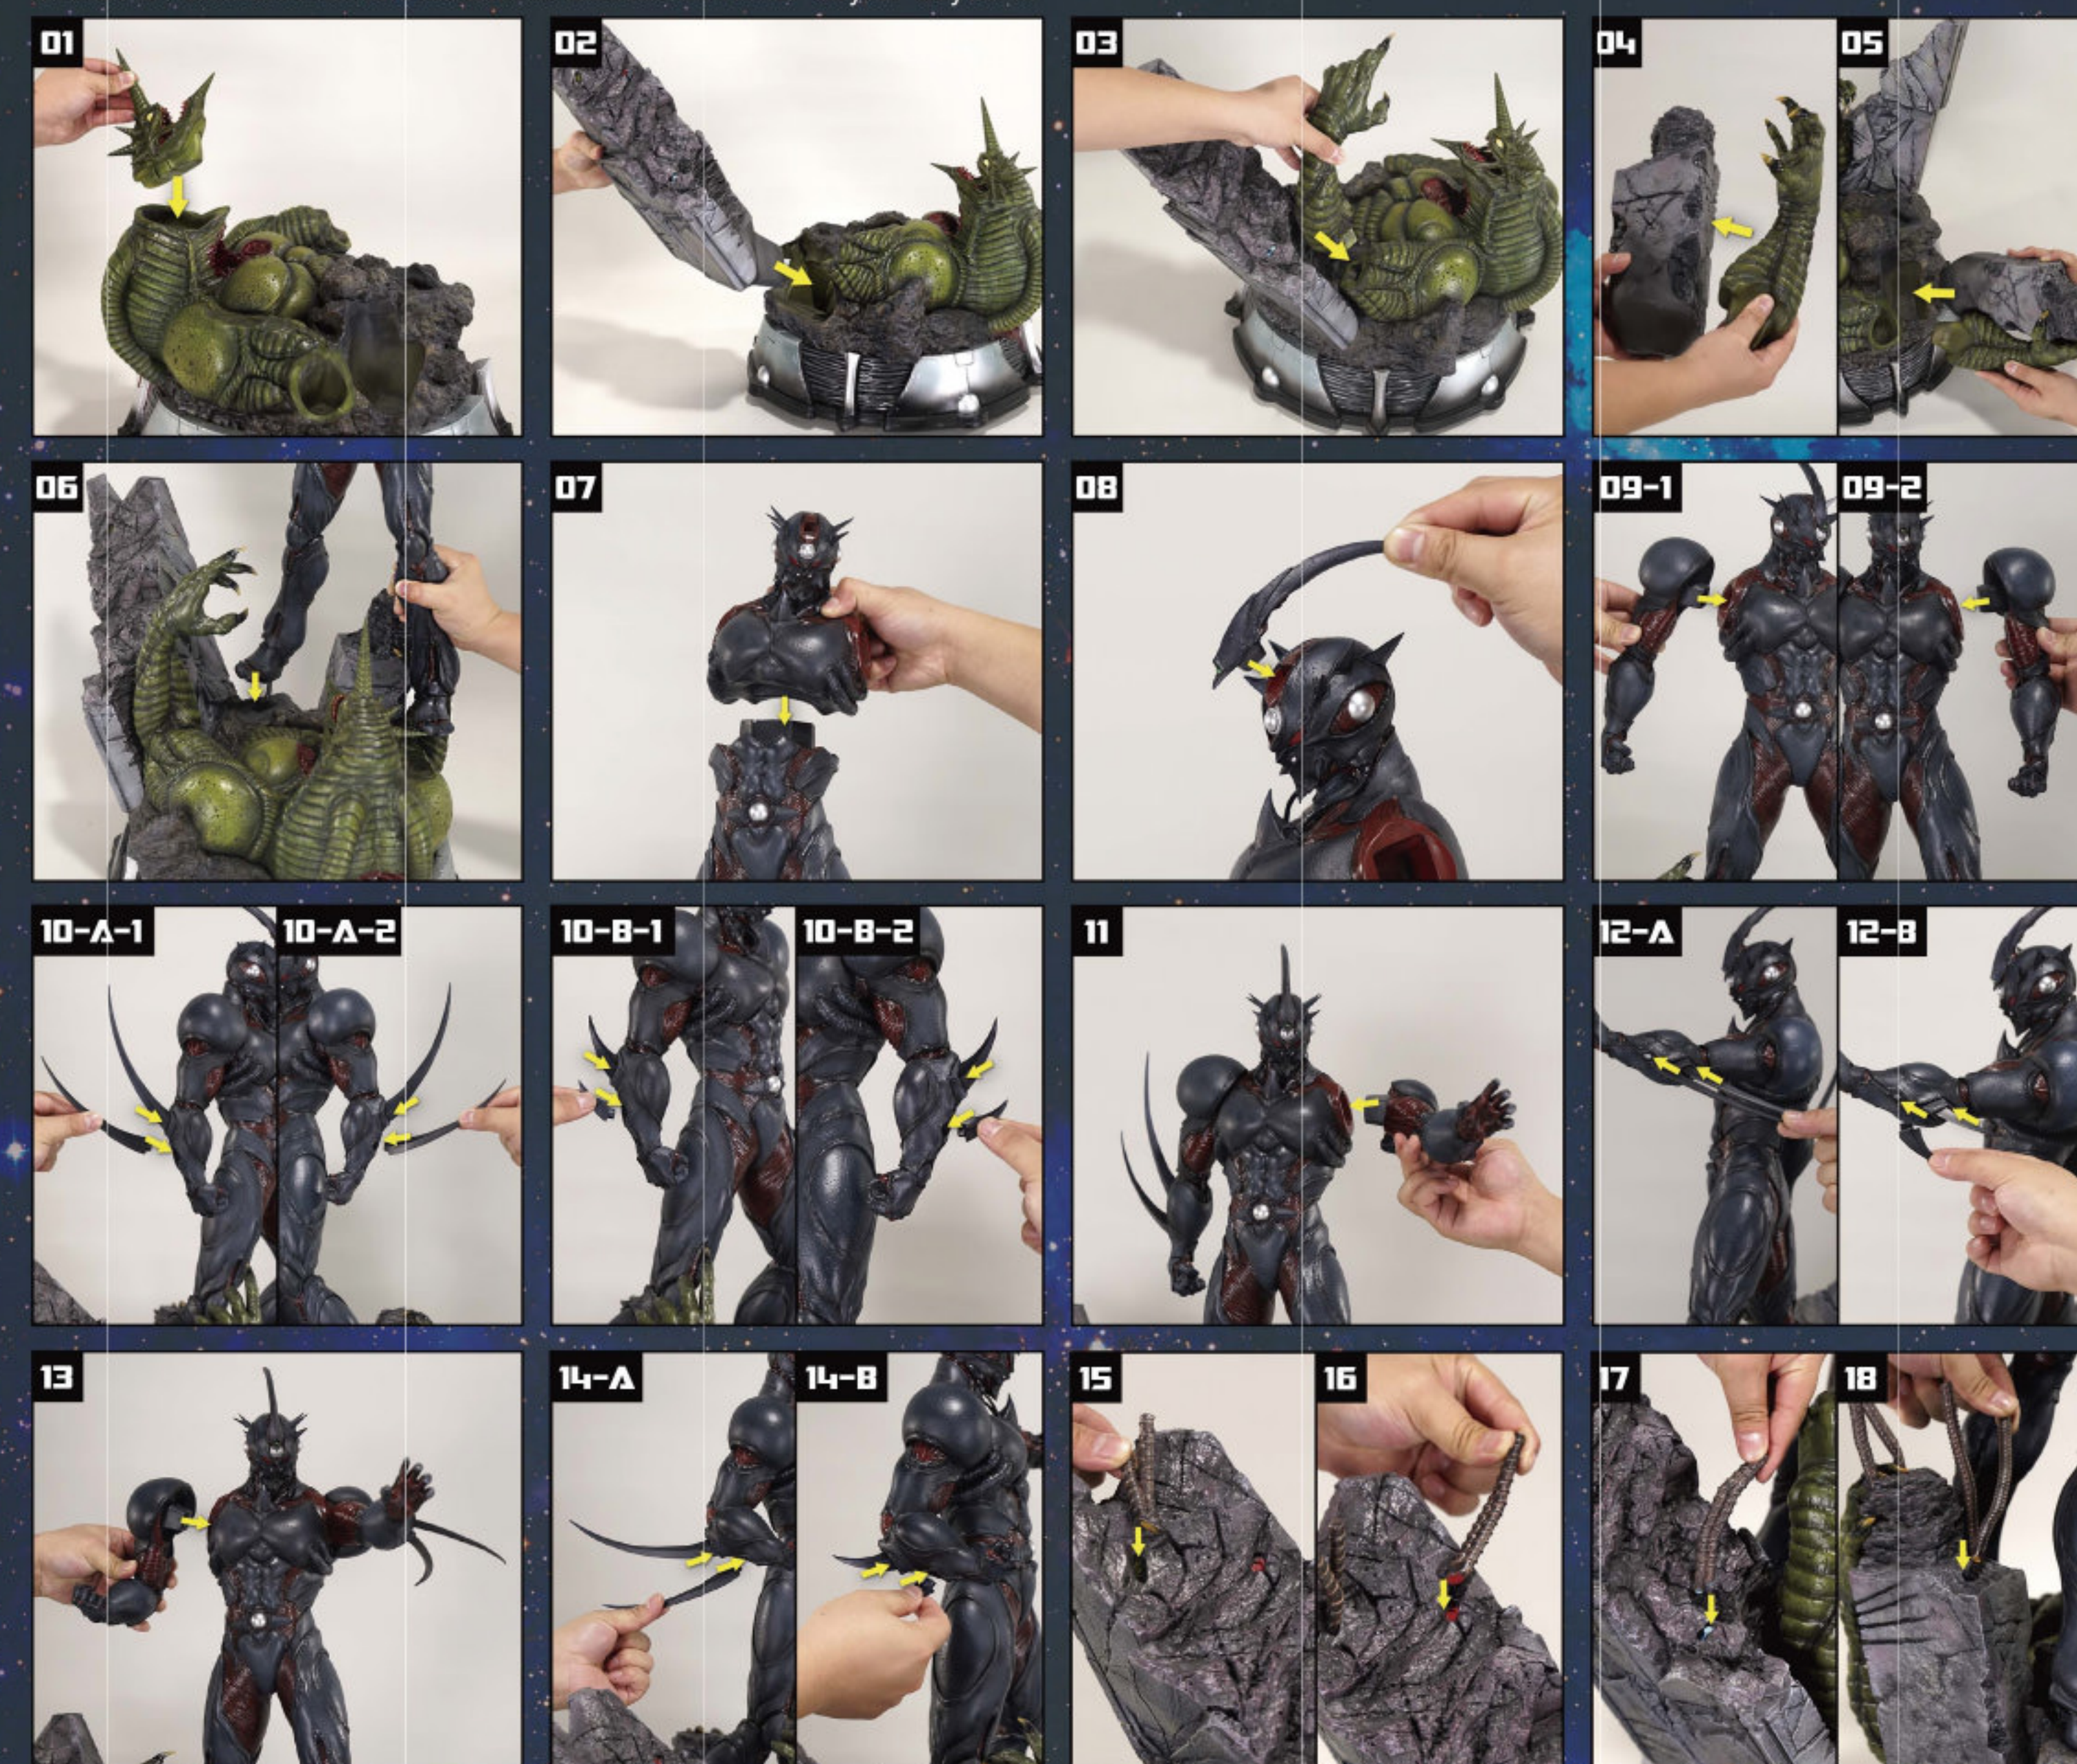

⚠ NOTICE
Due to the nature of the production, Small fragile part may changed shape direction during shipment. If it happend, we suggest to use a hair dryer to warm up the part for at least 45-60 seconds with a distance of 10 cm. Please adjust the part as you like and let it cool down.

商品は通常の輸送中に繊細な部品は小さな衝撃や気候の影響により多少変形する場合があります。もし部品の合わせに隙間がある場合、ドライヤーの熱風で45~60秒ほど温めながら手で押し付けてください。ドライヤーをパーツに近づけすぎないようにご注意ください。10 cm程度の距離を保つこととお勧めします。パーツが隙間なく密接するようになったら、ドライヤーの冷風で冷やして位置を定着させてください。



PRIME1
STUDIO
<https://www.prime1studio.co.jp>
<https://www.instagram.com/Prime1Studio>
<https://twitter.com/Prime1Studio>
<https://www.facebook.com/Prime1Studio>

© 高屋良樹 / KADOKAWA